INSTRUCTIONS FOR USE

PRODUCT NAME ReSolve® Locking Drainage Catheter


DESCRIPTION OF THE PRODUCT

The ReSolve Locking Drainage Catheter with locking pigtail and hydrophilic coating is a

radiopaque catheter with multiple side holes used for percutaneous drainage. The components of the catheter allow for introduction and placement using a trocar stylette or over-the-wire method. e ReSolve Locking Drainage Catheter may be packaged with the following components: • One (1) ReSolve Locking Drainage Catheter with locking pigtail (A), hydrophilic coating and

pigtail straightener (B) • One (1) Metal stiffening cannula (C)

- One (1) Flexible stiffening cannula (D)
- One (1) Trocar stylette (E)
- One (1) Dead end cap (G)
- One (1) Repositioning Tool (F)
- One (1) Marker band (H)

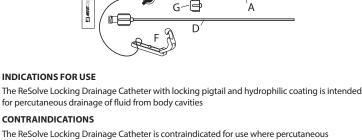

drainage catheterization is unacceptable. The ReSolve Locking Drainage Catheter is contraindicated for intravascular use. **PRECAUTIONS**

resterilization may also create a risk of contamination of the device and/or cause patient

• Follow universal precautions when inserting and maintaining this device. Due to the risk of bloodborne pathogens, healthcare professionals should always use standard blood and body fluid precautions in the care of all patients. Sterile technique should always be

· Read manufacturer's instructions prior to use. Contents of unopened, undamaged package are sterile.

· For single patient use only. Do not reuse, reprocess, or resterilize. Reuse, reprocessing, or resterilization may compromise the structural integrity of the device and/or lead to device failure, which in turn may result in patient injury, illness, or death. Reuse, reprocessing or

infection or cross-infection, including, but not limited to, the transmission of infectious disease(s) from one patient to another. Contamination of the device may lead to injury, illness, or death of the patient.

- Do not use after expiration date. · Store in a cool, dry place. WARNINGS $\bullet \ \, \text{The ReSolve Locking Drainage Catheter} \, \text{is not to be used to deliver nutritional supplements}.$ • The ReSolve Locking Drainage Catheter is not to be used in the biliary system.
- R Only Caution: Federal (U.S.A.) law restricts this device to sale by or on the order of a physician trained and/or experienced in the use of this device. ADVERSE REACTIONS*
- Septic shock Bacteremia

Superinfection · Bowel transgression · Pleural transgression

es for percutaneous nephrostomies.[Internet]. 2006. CIRSE.org.

· Catheter dislodgement

· Catheter occlusion

· Vascular injury

Hemorrhage

*Brountzos EN. Quality improvement guidelin http://cirse.org/files/File/05_qig.pdf. Accessed 04/11/13.

2003;14:S277-S281.

- Wallace MJ, et al. Quality improvement guidelines for percutaneous drainage/aspiration of abscess and fluid collections. J Vasc Interv Radiol. 2010;21:431-435. amchandani P, et al. Quality improvement guidelines for percutaneous nephrostomy. J Vasc Interv Radiol.
- **INSTRUCTIONS FOR USE OPTION 1:** DIRECT PLACEMENT USING TROCAR STYLET
- water or saline. Keep the distal portion of the catheter wet during placement. WARNING: DO NOT wipe catheter with dry gauze or any solvents because it may damage the catheter coating.

2. Slide pigtail straightener along distal portion of catheter to straighten curve prior to placing metal stiffening cannula into the catheter. Place the metal stiffening cannula into the catheter and tighten the Luer lock fittings. See Figure 1.

rotating the arm proximally to the point of resistance.

before connecting the drainage tubing or dead end cap.

1. Wet the distal portion of the ReSolve Locking Drainage catheter prior to use with sterile

3. Remove the paper spacer from the trocar stylette. Advance the trocar stylette through the metal stiffening cannula and tighten the Luer lock fittings. See Figure 2.

Figure 2

Figure 1

7/





Figure 3 Note: If the catheter needs to be repositioned, unlock the suture locking mechanism by







Figure 5

5. Place catheter/cannula assembly over appropriate guide wire and advance into the fluid collection site. The catheter accommodates a 0.038" (0.97 mm) wire. See Figure 6.

Figure 6



Precaution: Do not rotate the suture locking mechanism beyond the point of resistance. Rotating the suture locking mechanism beyond the point of resistance will not release the


Caution: Consult accompanying documents. Single use.

Do not resterilize

MERITAEDICAL www.merit.com

- 4. Remove pigtail straightener from catheter prior to insertion. 5. Place the catheter/cannula/trocar assembly into the fluid collection site using standard insertion technique. Note: Placement should be confirmed with diagnostic imaging. 6. After placement is confirmed, remove the trocar stylette and stiffening cannula. 7. To engage the suture locking mechanism: Pull the suture until desired pigtail is formed. Rotate the suture locking mechanism distally to hold the suture in place. See Figure 3. 4
 - Figure 4 9. The ReSolve Locking Drainage Catheter is now ready to be connected to appropriate drainage bag, tubing or dead end cap. WARNING: If using alcohol to clean the catheter hub, allow sufficient time for alcohol to dry

WARNING: DO NOT over tighten the connection between the drainage catheter and



1. Remove the stiffening cannula and trocar stylette assembly from catheter.

4. Remove pigtail straightener from catheter prior to insertion.

rotating the arm proximally to the point of resistance.

suture to allow the pigtail to straighten upon removal.

CATHETER EXCHANGE, REPOSITIONING OR REMOVAL 1. Disconnect catheter from drainage bag, tubing or dead end cap. 2. To release the pigtail loop choose one of the following options:

Using the Repositioning Tool align the opening of the

suture to allow the pigtail to straighten upon removal.

on or before 90 days post placement.

THE CATHETER BE ATTACHED TO THE PATIENT'S CHART.

exchange or skin closure.

drainage tubing or dead end cap.

protocol of the physician.

Gently squeeze together.

proximal position.

Option 2:

maintenance


Note: Placement should be confirmed with diagnostic imaging.

 ${\it 6. After placement is confirmed, remove the stiffening cannula and guide wire.}\\$ 7. To engage the suture locking mechanism: Pull the suture until desired pigtail is formed. Rotate the suture locking mechanism distally to hold the suture in place. See Figure 7.

Figure 7 Note: If the catheter needs to be repositioned, unlock the suture locking mechanism by

Precaution: Do not rotate the suture locking mechanism beyond the point of resistance. Rotating the suture locking mechanism beyond the point of resistance will not release the

8. Once placement is confirmed, and the suture locking mechanism has been rotated to the most distal position, press the suture locking mechanism into the hub to secure it. The



WARNING: DO NOT over tighten the connection between the drainage catheter and

Note: A flush regimen should be designed for the circumstances of each patient and the

Note: Instruct patient or other healthcare personnel in appropriate device function and/or

round section of the

• Bring the flat back of the Repositioning Tool around the catheter hub. • Remove the Repositioning Tool and rotate the suture locking mechanism to the most

Repositioning Tool in line with the handle of the suture locking mechanism.

For exchange or removal only, cut the hub off the drainage catheter and sever suture. This will release the suture and the pigtail loop. WARNING: The suture will no longer be secured to the catheter. Take care to remove both the suture and catheter.

3. For catheter exchange or if access is to be maintained, advance appropriate guide wire through catheter; using diagnostic imaging to confirm guide wire placement. Guide wire will maintain access to drainage site. To ease guide wire placement, a stiffening cannula may WARNING: When long-term use is indicated, it is recommended that indwelling time not exceed 90 days. The ReSolve Locking Drainage Catheter should be evaluated by a physician

4. Carefully remove the ReSolve Locking Drainage Catheter. Proceed with either catheter

ATTENTION ATTENDING PHYSICIAN: IF PATIENT WILL NOT BE FOLLOWED UP BY YOU, IT IS RECOMMENDED THAT THE "INSTRUCTIONS FOR USE" OR THE SECTION ON HOW TO REMOVE

- Caution: Federal (USA) law restricts this device to sale by or on the R_X Only order of a physician.
- MAX GUIDE WIRE
- Non-pyrogenic Do not use if package is damaged STERILE Sterilized using ethylene oxide Maximum diameter guide wire



402955005EN_002 2020-04-20

C €₂₇₉₇

Manufacturer: Merit Medical Systems, Inc. 1600 West Merit Parkway South Jordan, Utah 84095 U.S.A. 1-801-253-1600 U.S.A. Customer Service 1-800-356-3748